Journal of Manufacturing Engineering, 2009, Vol. 4, Issue 4, pp 293-297



# SIMULATION IN MEMS OF THE STATUS OF SPECIFIC GRAVITY OF URINE AND ITS CORRELATION IN DATA MINING

## \*T K Basak<sup>1</sup>, T Ramanujam<sup>2</sup>, Arpita Gupta<sup>3</sup> and Poonam Goyal<sup>4</sup>

<sup>1</sup>Director, Krishna Engineering College, Mohan Nagar, Ghaziabad. Uttar Pradesh, India. - 201007 <sup>2,3,4</sup> Department of Electronics and Communication Engineering, Krishna Engineering College, Mohan Nagar, Ghaziabad. Uttar Pradesh, India. - 201007

# ABSTRACT

The status of specific gravity of urine in respect of parenchymal lesion involved in bacterial infection is of great medical importance for the treatment of the subject. The conclusion of the doctor is based on the accurate results in respect of the status of the specific gravity of urine. Mems is a effective and accurate tool for the measurement of the specific gravity of the liquid and thus the simulated results of the MEMS is of importance in respect to the diseases like nephropathy and parenchymal lesion. The trend of the diseases can be correlated with the simulated output for which classification is done in the data mining software DTREG for helping the physicians so that they can prescribe the treatment of the subject in a precise manner.

**Keywords:** Simulation of MEMS, Analysis of Specific Gravity of Urine and Renal Diseases, Data Mining.


# 1. Introduction

For the diagnosis of different diseases like nephropathy and parenchymal lesion involved in bacterial infection, it is required to measure the specific gravity of urine [1, 2, and 3]. The existing method of measuring specific gravity of urine is time consuming, and involves possibility of human error. Thus we have introduced a new method to measure specific gravity of urine using MEMS. The phenomenon of cavity resonator is being used in our method. The concentration of solute in urine (specific gravity of the urine) can be measured by micro Electro Mechanical System (MEMS). For minimum specific gravity, the electrodes of MEMS will vibrate with maximum amplitude and thus the amplitude of the vibration of electrode is functionally related to specific gravity which is the underlying principle of MEMS for the measurement of specific gravity of urine in the context of this paper [4].

In density measurement methodology, the higher the weight of the fluid, the lower the resonant frequency of the filled tube. The density or specific gravity sensor employs a chip level, vacuum packaged, and resonating silicon tube. While filled with a fluid, the tube is driven into resonance electrostatically and its motion sensed capacitively. Data obtained from the sensor is fed to software for further analysis of urine samples.

# 2. Existing System

The Existing system is a manual process which consumes weeks or months to test the urine from micro array expression data. In this system the diagnosis is based on various data like symptoms observations, laboratory data, bio statistic information, data base of the patient [5, 6, 7, 8]. The whole process is represented in the form of the block diagram as shown in Fig 1.

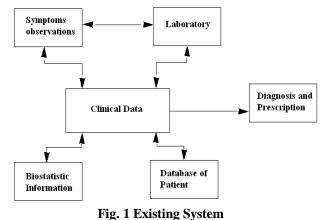

Courtesy: Proceedings of 3<sup>rd</sup> National Conference on Recent Trends in Instrumentation Applications -National Engineering College, K. R. Nagar, Kovilpatti – 628 503, Tamilnadu, India

293

\*Corresponding Author- E-mail: tkb20042001@yahoo.co.in

#### Journal of Manufacturing Engineering, 2009, Vol. 4, Issue 4, pp 293-297

diagnosis is based on various data like symptoms observations, laboratory data, bio statistic information, data base of the patient Bergamo F Et al. [5], Jorgeiisen K. Et al. [6], Albright F Et al.[7], Rohbins S. L, Kumar V. et al. [8].

#### Draw Backs of the Existing System

- i. Time consuming
- ii. Uncertainty in Decision Making
- iii. Possibility of human errors
- iv. Generates Bewildering amount of data

## 3. Proposed System

The proposed system is an automatic system which computes and takes decision automatically J. B. Tenenbaum Et al. [9], T.K.Basak Et al. [10]. Two sets of data have been made. One set of data has been used to train the system. After the system is trained then the system is tested with the other set of data. Later the system can take decision for any unknown data automatically. The block diagram of the system is shown in Fig. 2.

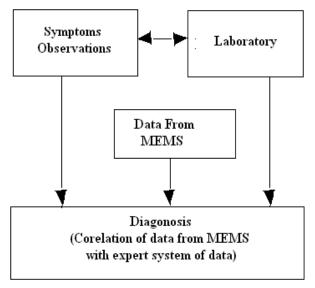


Fig. 2 Proposed System

#### Advantages of Proposed system


- i. Model produced high quality of output for urine test.
- ii. Produce reliable performance estimates.
- iii. Allow to apply models to unseen patients

#### **3.1 MEMS**

A capacitive sensor performs best with small gaps between electrodes. For micro machines, close spacing leads to squeeze film damping and molecular interaction during motion. For a resonant device, extensive damping results in low Q values (resonator quality factor) or poor signal-to-noise ratio. Vacuum packaging of the micro tube is employed to overcome this problem along with a compatible electrical lead transfer design. This has been accomplished using vacuum wafer-to-wafer bonding methods. From Mems measurement of specific gravity of urine was done by comparing its value with standard curve obtained in simulation of Mems D. Sparks, Et al. [4].

# 3.2 Resonant frequency of electrode of MEMS with gain

For minimum specific gravity, the electrodes of MEMS will vibrate with maximum amplitude and thus the amplitude of the vibration of electrode is functionally related to specific gravity. Both these phenomena have been simulated by MATLAB 7.0 T K Basak, Et al. [11].



## Fig. 3 Sample Closed Loop Transfer Function of Simulation of MEMS

The sample closed loop transfer function of simulation of MEMS is as shown in Fig. 3.

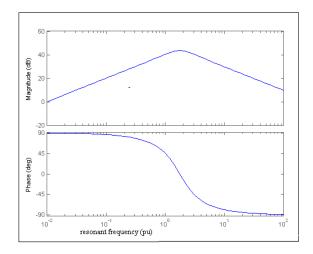


Fig. 4 Relation of Frequency Vs Gain

#### 3.3 Relation of specific gravity of liquid and output voltage of MEMS

Different curves of various resonant frequencies representing different urine samples have been simulated in MATLAB. The plot between gain and frequency is shown in Fig.4. Data obtained from MATLAB are decoded so that it can be fed to software

© SME

for further analysis and correlation with the data of urine sample obtained from laboratory corresponding to the status of the subject. As the specific gravity of the liquid increases, the density of the liquid also increases and thus the mass of the liquid increases Paul S. Et al. [12], Nicolas Demaurex Et al. [13]. With different specific gravity i.e. different concentration of liquid the output voltage of Mems will vary according to the curve shown in Fig 5.






Fig. 5 Relation of Specific Gravity of Liquid and Output Voltage of MEMS

1 per unit voltage = 1V

1 per unit specific gravity = 1.05 gm/cc

## 3.4 Relation of frequency and Q factor





1 per unit Q-factor = 10 1per unit frequency = 10 kHz

Different curves of various resonant frequencies representing different urine samples have been simulated in MATLAB.

A relation between frequency and Q factor=  $(\Delta f/f) = (\Delta m/m)$  has been plotted after studying different curves where  $\Delta f$  is change of frequency corresponding 3db difference with max value corresponding to f. The relation obtained is as shown below in Fig 6.

# 3.5 Relation of mass of the liquid and resonant frequency

The relation was obtained by studying the result from Matlab and is shown below in Fig 7.




Fig. 7 Relation of Mass of the Liquid and Resonant Frequency

1 per unit resonant frequency= 10 KHz

1 per unit specific gravity = 1.05 gm/cc

#### 3.6 Matlab simulation in renal disorder

The curves have been simulated in Matlab Simulink 7.0. In this we have simulated the curves related to specific gravity of the urine related to bacterial infection and this simulation is in agreement with the clinicalvalues.

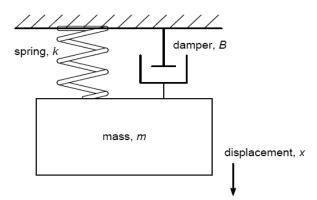


Fig. 8 Representation of Silicon Tube Resonator

The silicon tube resonator can be represented by equivalent mechanical configuration shown in Fig.8.

A typical block diagram involved in simulink 7.0 is shown below in Fig. 9

© SME




Fig. 9 Block Diagram in Simulink 7.0

The transfer function of Matlab simulation is given by to equation below

$$G(\mathbf{s}) H(s) = \frac{1}{m \cdot s^2 + B \cdot s + k}$$

The graph shows the different stages of status of bacterial infection with time. Specific gravity of urine if regularly checked is an important parameter in the diagnosis of diseases J. B. Tenenbaum Et al. [9], Rivera F, Et al. [14], Lawton JM, Et al. [15], T. K. Basak Et al. [16]. We have simulated the curves in normalized way for projecting the status of the subject suffering from repeated bacterial infection T. K. Basak, Et al. [17], Basak T.K. Et al. [18], Betz. A, Et al. [19], Basak T. K., Et al. [20], Basak T. K., Et al. [21].

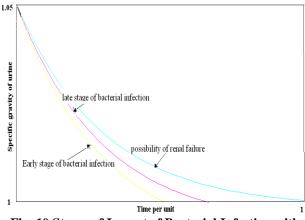


Fig. 10 Stages of Impact of Bacterial Infection with Time

1 per unit time = 2 Years

There is a possibility of renal failure with repeated and very late bacterial infection as shown in Fig 10.

# 4. Data Mining

Parenchymal lesion may be caused by repeated bacterial infection in urinary tract. The status of diseases associated with bacterial infection has been classified in data mining through the use of software DTREG Pascal

#### Journal of Manufacturing Engineering, 2009, Vol. 4, Issue 4, pp 293-297

Houillier, Et al. [22], J. A. Costa Et al. [23]. Data mining is a powerful statistical analysis program that generates classification and regression decision trees that model data and can be used to predict values. Data mining has been done by the software DTREG which is a robust application that is installed easily on any Windows system. DTREG reads Comma Separated Value (CSV) data files that are easily created from almost any data source. Through DTREG the classification of trees has been done through a particular option (single tree mode) present in the software where the target variable being predicted is categorical and Regression.

## 5. Result

The results of data mining associated in repeated bacterial infection in the context of the status of the kidney has been done and the results indicate that there is possibility of renal failure for repeated late bacterial infection when the specific gravity is greater than 1.029. When the specific gravity is less than 1.029 and approaching towards 1 then there is no possibility of renal failure. Table 1 shows the status of the subject with duration of infection linked with specific gravity of urine.

# 6. Conclusion

The status of kidney with repeated bacterial infection has a great impact on the physiological condition of the subject. In this respect the status of kidney of the subject should be of great concern related to repeated bacterial infection.

mining			
Time (Month)	Specific Gravity	Diseases	Mis classification
<=17.2	<b>⊳1.00</b> 9	Late BI*	60.76%
<=17.2	<=1.009	Late BI*	30.77%
<= <b>11.6</b>	<b>≺=1.00</b> 9	Early BI*	0%
> <b>11.6</b>	<b>≺=1.00</b> 9	Late BI*	0%
<=17.2	>1.009	Renal Failure	53.03%
<= <b>13.6</b>	≻ <b>1.00</b> 9	Renal Failure	61.4%
>13.6	<b>&gt;1.00</b> 9	Renal Failure	0%
<b>&lt;= 10</b>	<b>≻1.00</b> 9	Late BI*	66.67%
>10	> <b>1.00</b> 9	Late BI*	<b>50</b> %
<= 10	<b>&lt;</b> =1.03	Early BI*	27.27%
<b>&lt;= 10</b>	≻ <b>1.0</b> 3	Renal Failure	53.57%
> <b>10</b>	<=1.029	Late BI*	30.77%
>10	>> <b>1.02</b> 9	Renal Failure	0%

Table 1: Status of various diseases in Data

\* BI- Bacterial Infection

#### Journal of Manufacturing Engineering, 2009, Vol. 4, Issue 4, pp 293-297

# References

- 1. Hein Van Poppel (2000), "Nephron Sparing Surgery in Renal Cell Carcinoma", Clinical Urology, Vol. 26(4), 342-353.
- Leiinon E J, Lcmann J and Litzow J R (1966), "The Effects of Diet and Stool Composition on the Net Exte Acid Balance of Normal Subjects", I. Clin. Invest, Vol. 45, 1601-1607.
- 3. Burton R F Acid and Bose Exretion (1980), "Assessment Krelationships To Diet 81 Urine Composition", Comp. Biochemistry, Physiol, Vol.66a, 371-375.
- Sparks D, Massoud-Ansari, Straayer M, Smith R, Schneider R, Cripe J, Zhang Y, Meng G (2002) "A Density / Specific Gravity Meter Based on Silicon Microtube Technology", Proceedings Sensors Expo, Fall 2002, Boston, MA 2002, 171-176.
- Bergamo F and Dikstein S (1955). "The Relationship Behveen Spectral Shifts and Structural Changes in Uric Acids and Related Compounds" J. Ain Chem. Soc. Vol 77,691-696.
- Jorgeiisen K (1957), "Micrometric Determination of the Net Excretion of Acidbase in Urine". Scand. I. clin-lab. Invest. Vol 9,287-291
- Albright F and Bauer W (1929), "The Action of Sodium chloride, Ammonium Chloride, And Sodium Bicarbonate 181. J.clin. Invest. Vol. 7, 465-486.
- Rohbins S L, Kumar V (1987) "Basic Pathology", The Kidney and Its Collecting System, edited by Cotran RS, Philadelphia, W.B. Saunders, 4th ed, 457–491
- Tenenbaum J B, De Silva V and Langford J C, "A Global Geometric Framework for Dimensionality Reduction" Vol.290(no.5500)2319-2323,
- Basak TK, Ramanujam T, Cyrilraj V, Rahul Dayal, Arpita Gupta, Prachi Mohan Kulshrestha and Poonam Goyal (2008) "Measurement Of Specific Gravity Of Urine Using MEMS And Data Mining". VCAN Chennai
- Tapas K Basak, Suman Halder, Madona Kumar, Renu Sharma and Bijoylaxmi Midya(2005) "A Topological Model Of Biofeedback Basedon Catecholamine Interactions". Theoretical Biology And Medical Modelling, 2:11
- Paul S Uster and David W Deamer, (1985). "pH Dependent Fusion Of Liposomes Using Titrahle Polycatioiis", J. Am. Chem. Soc. Vol 24,1,1985

- 13. Nicolas Demaurex (2002). "pH Homeostasis of Cellular Organelles". News in Physiological Sciences, Vol. 17, No. 1, 1-5
- 14. Rivera F, Vazmediano C, Gonzalez Lopez L, Carrano A, and Blanco J (1985), "Subacute renal failure in diabetic nephropathy due to endocapillary glomerulonephritis and cholesterol embolization" Journal of nephrology Vol 21(4),615-620
- Lawton JM, Conway LT, Crosson JT, Smith CL, Abraham (1985), "Acute oxalate nephropathy after massive as ascorbic acid administration" Arch Intern Med, 145(5):950-1
- Basak T K (1996), "pH dependent transduction in renal function regulation", 18th Annual International Conference of the IEEE Engineering in Medicine and Biology Society, Amsterdam.
- 17. Basak T K, Ramanujam T, Cyrilraj V, Gunshekharan Asha Khanna G, Deepali Garg, Poonam Goyal and Arpita Gupta (2009), "pH Homeostasis of a Biosensor in Renal Function Regulation Linked with UTI" Vol. 105, (6), 127-134.
- Basak T K (1991), "Entropy Transduction on Photoinduction", Proceedings of the 13th Annual International Conference, IEEE (EMBS), part -4/5, 1534-1535.
- 19. Betz A, Hofsteangc J and Kr stonc S R, (1992), "pH Dependence of the interaction of hirudin with thrombin", .I. Am.chem. Society (Bio-chemistry) Vol.31, (4), 1168-1172.
- Basak T K and Islam R (1993), "Role of Scnwry Hormones in Estimation of Blood Pressure Transduction", Proceedings of 15th Annual International Conference, IEEE (EMBS), Vol 3.
- 21. Basak T K, and Dutla J(1994), "pH Dependence Of The Interactions In Blood Pressure Transduction" Proceedings Of The 16th Annual International Conference Of IEEE (EMBS), Vol.1.
- 22. Pascal Houillier, Pascale Borensztein, Maurice Bichara, Michel Paillard, and Alian Prigent (1992), "Chronic Neutral Phosphate Supplementation Induces Sustained, Renal Metabolic Alkalosis". Kidney International, Vol.41, 1182-1191.
- 23. J. A. Costa and A. O. Hero, (2001) "Classification Constrained Dimensionality Reduction". In IEEE International Conference on Accoustic Speech, and Signal Processing, volume 5, 1077-1080.